



Stand-on Floor Scale

USER MANUAL **MS4910**




Please keep the instruction manual at hand and follow instruction for use.

CONTENTS

I. Explanation of Graphic Symbols on Label/Packaging	4
II. Copyright Notice	6
III. Safety Notes	7
A. General Information	7
B. EMC Guidance and Manufacturer's Declaration	12
IV. Installation	18
A. Assembly	18
B. Inserting Batteries	21
C. Using Adapter	24
D. Attaching Height Rod to Column	25
E. Attaching Thermal Printer	29
V. Indicator	32
A. Indicator and Key Functions	32
B. Display layout	33
VI. Using Device	34
A. Basic Operation	34
B. Hold	34
C. BMI	35
D. Tare	36
E. Pre-Tare	36
F. Print	40
VII. Device Setup	41
A. Setting Time & Date	41
B. Device Setup	42
VIII. Setup USB Connection to PC	44
IX. Wireless Connection	47
X. Troubleshooting	48
XI. Product Specifications	51
A. Device Information	51
B. Power Adapter Standards	52
XII. Declaration of Conformity	55

I. Explanation of Graphic Symbols on Label/Packaging

Text/Symbol	Meaning
	Caution, consult accompanying documents before use
	Separate collection for waste of electrical and electronic equipment, in accordance with Directive 2002/96/EC. Do not dispose of device with everyday waste
	Name and address of device manufacturer, and year/country of manufacture
	Carefully read user manual before installation and usage, and follow instructions for use.
	Medical electrical device, Type B applied part
	Medical electrical device, Type BF applied part
REF	Device catalogue number / model number
EC REP	Name and address of authorized representative in the European Union
MD	Device is a medical device. Text indicates device category type
LOT	Manufacturer's batch or lot number for device
SN	Device's serial number
UDI	Device's Unique Device Identifier
e	Verification Scale Interval. Value expressed in units of mass. Used to classification and verification of an instrument.

	Device conforms to (EU) 2017/745 Regulation on Medical Devices. Fourdigit number is identifier for medical device Notified Body
	Device complies with EC directives (verified models only)
	M : Conformity label in compliance with Directive 2014/31/EU for non-automatic weighing instruments 20 : Year in which conformity verification was performed and the CE label was applied. (ex: 16=2016) 0122 : Identifier for metrology Notified Body
	Device is a Class III scale in compliance with Directive 2014/31/EU (verified models only)
	Name and address of entity importing device (if applicable)
	Name and address of entity responsible for translating Information For Use (if applicable)
CON.	Event counter confirming how many times device has been calibrated (if applicable)
	Device conforms to Taiwan National Communications Commission(NCC) approval
	Device conforms to U.S. Federal Communications Commission regulations
	Device complies with UK non-automatic weighing instruments regulations 2016 (verified models only) M : Conformity label in compliance with Non-automatic Weighing instruments Regulations 2016 20 : Year in which conformity verification was performed and the UKCA label was applied. (ex: 20=2020) 8506 : Identifier for metrology approved body
	Device complies with all UK applicable product legislation
	Device's polarity of power.

"In case of differences, icon on device itself takes precedence"

II. Copyright Notice

Copyright Notice

Charder Electronic Co., Ltd.

No.103, Guozhong Rd., Dali Dist., Taichung City 41262 Taiwan

Tel: +886-4-2406 3766

Fax: +886-4-2406 5612

Website: www.chardermedical.com E-mail:

info_cec@charder.com.tw

Copyright© Charder Electronic Co., Ltd. All rights reserved.

This user manual is protected by international copyright law. All content is licensed, and usage is subject to written authorization from Charder Electronic Co., Ltd. (hereinafter Charder) Charder is not liable for any damage caused by a failure to adhere to requirements stated in this manual. Charder reserves the right to correct misprints in the manual without prior notice, and modify the exterior of the device for quality purposes without customer consent.



Charder Electronic Co., Ltd.
No. 103, Guozhong Rd., Dali Dist.,
Taichung City, 41262 Taiwan

III. Safety Notes

A. General Information

Thank you for choosing this Charder Medical device. It is designed to be easy and straightforward to operate, but if you encounter any problems not addressed in this manual, please contact your local Charder service partner.

Before beginning operation of the device, please read this user manual carefully, and keep it in a safe place for reference. It contains important instructions regarding installation, proper usage, and maintenance.

Intended Purpose

This medical device is designed to be used in accordance with national regulations, to measure weight within specifications, for weight-related usage by professionals.

Clinical Benefit

Measurement results can be used by professionals to diagnose (and monitor) weight-related issues.

Intended medical indications/contraindications

Measurement: patient's body weight. No known contraindications to measurement of body weight.

Intended patient profile

- (a) Age: no restrictions
- (b) Weight: no restrictions within device weight capacity
- (c) Patient Conditions: require measurement of body weight.
Able to stand independently without support.

Intended user profile

- (a) At least 20 years old
- (b) Minimum knowledge:
 - To be able to read at a high-school level and understand Arabic numerals (e.g. 1, 2, 3, 4...)
 - Basic hygiene knowledge
 - Trained in device's operation
 - Read the instruction manual
- (c) Language
 - Able to read the language of instruction manual and on-screen instructions
- (d) Qualifications
 - No special certifications or qualifications required

Residual Risk Evaluation

- (a) All foreseeable risks have been evaluated and considered acceptable. Generally speaking, the most likely risk caused by incorrect usage of the device is less accurate measurement (or inability to use device to acquire measurement), which does not pose imminent physical risk to patient or user.
- (b) Benefit-risk ratio is considered acceptable. Stand-on floor scales are an important option for measuring patients. Usage of device is unlikely to result in harm to user or patient.

General Handling

- Device should be placed on stable, flat, solid, non-slippery surface.
- Usage on soft surfaces (ex: carpet) may result in inaccurate results.
- Ensure all parts are properly locked and tightened before operating the device.
- Device is intended to measure one subject at a time.

Safety Instructions

Before putting device into use, please read this user manual carefully. It contains important instructions for installation, usage, and maintenance of device.

The manufacturer shall not be liable for damages caused by failure to heed the following instructions:

- Batteries should be kept away from children. If swallowed, promptly seek medical assistance.
- Expected service life: 5 years.
- Always comply with appropriate regulations when using electrical components under increased safety requirements.
- Improper installation will render the warranty null and void.
- Ensure voltage marked on power supply matches mains power supply.
- The device is intended for indoor use only.
- Observe permissible ambient temperatures for use
- Device meets requirements for electromagnetic compatibility. Do not exceed the maximum values specified in the applicable standards.

Environmental

- All batteries contain toxic compounds; batteries should be disposed of via designated competent organizations. Batteries should not be incinerated.

Cleaning

- Device surface should be cleaned using alcohol-based wipes. Corrosive cleansing liquids should not be used. Pressure-washers should not be used.
- Do not use large amounts of water when cleaning the device, as it may cause damage to the internal electronics.
- Always disconnect device from mains power before cleaning.

Maintenance

- Please contact your local Charder distributor for regular maintenance and calibration, regular checking of accuracy is recommended; frequency to be determined by level of use and state of device.

Warranty/Liability

- If Charder is responsible for a fault or defect present upon receipt of the unit, Charder shall either repair the fault, or supply a replacement unit. Should the repairs or replacement delivery fail, statutory provisions shall be valid. The period of warranty shall be two years, beginning on the date of purchase. Please retain your receipt as proof of purchase.
- No responsibility shall be accepted for damage caused through any of the following reasons: unsuitable or improper storage or use, incorrect installation or commissioning by the owner or third parties, natural wear and tear, changes or modifications, incorrect or negligent handling, chemical, electrochemical, or electrical interference, unless damage is attributable to negligence on the part of Charder.
- This device does not contain any user-maintained parts. All maintenance, technical inspections, and repairs should be conducted by an authorized Charder service partner, using original Charder accessories and spare parts. Charder is not liable for any damages arising from improper maintenance or usage. Dismantlement of the device will void the warranty.

Disposal

- This product is not to be treated as regular household waste, but should be taken to a designated collection points for electronics. Further information should be provided by local waste disposal authorities.



Warning

- Only the original adapter should be used with the device. Using an adapter other than the one provided by Charder may cause malfunction.
- Do not touch the power supply with wet hands.
- Do not crimp the power cable, and avoid sharp edges.
- Do not overload extension cables connected to the device.
- Route cables carefully, to avoid tripping.
- Keep device away from liquids.
- Do not remove the plug by yanking on the cable.
- Use only a correctly wired (100-240VAC) outlet, and do not use a multiple outlet extension cable.
- Do not under any circumstances dismantle or alter the device, as this could result in electric shock or injury as well as adversely affect the precision of measurements.
- Do not place the device in direct sunlight, or in close proximity to an intense heat source. Excessively high temperatures may damage the internal electronics.

Incident Reporting

- Any serious incident that has occurred in relation to the device should be reported to the manufacturer, EU representative (if device is used in EU member state), and competent authority of user/subject's member state.

B. EMC Guidance and Manufacturer's Declaration

Guidance and manufacturer's declaration-electromagnetic emissions		
The product is intended for use in the electromagnetic environment specified below. The customer or the user of the product should assure that it is used in such an environment.		
Emission test	Compliance	Electromagnetic environment-guidance
RF emissions CISPR 11	Group 1	The product uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class A	The product is suitable for use in all establishments other than domestic and those directly connected to a low voltage power supply network which supplies buildings used for domestic purposes.
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations /flicker emissions IEC 61000-3-3	Compliance	

Guidance and manufacturer's declaration-electromagnetic immunity			
The product is intended for use in the electromagnetic environment specified below. The customer or the user of the product should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment-guidance
Electrostatic discharge(ESD) IEC 61000-4-2	<u>±8 kV contact</u> <u>±2 kV, ±4 kV,</u> <u>±8 kV, ±15 kV</u> <u>air</u>	<u>±8 kV contact</u> <u>±2 kV, ±4 kV,</u> <u>±8 kV, ±15 kV</u> <u>air</u>	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%
Electrical fast transient/burst IEC 61000-4-4	+ 2kV for power supply lines	+ 2kV for power supply lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	<u>+ 1kV line(s) to line(s)</u> <u>+ 2kV line(s) to earth</u>	<u>+ 1kV line(s) to line(s)</u> <u>+ 2kV line(s) to earth</u>	Mains power quality should be that of a typical commercial or hospital environment.
Voltage Dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	<u>0% UT for 0,5 cycle</u> <u>0% UT for 1 cycle</u> <u>70% UT(30% dip in UT) for 25cycles</u> <u>0% UT for 5 s</u>	<u>0% UT for 0,5 cycle</u> <u>0% UT for 1 cycle</u> <u>70% UT(30% dip in UT) for 25cycles</u> <u>0% UT for 5 s</u>	Mains power quality should be that of a typical commercial or hospital environment. If the user of the product requires continued operation during power mains interruptions, it is recommended that the product be powered from an uninterruptible power supply or a battery.

Power frequency(50, 60 Hz) magnetic field IEC 61000-4-8	<u>30 A/m</u>	30 A/m	The product power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
NOTE UT is the a.c. mains voltage prior to application of the test level.			

Guidance and manufacturer's declaration-electromagnetic immunity			
The product is intended for use in the electromagnetic environment specified below.			
The customer or the user of the product should assure that is used in such and environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment-guidance
Conducted RF IEC 61000-4-6	3 Vrms 150 KHz to 80 MHz <u>6 V in ISM bands</u> <u>between 0,15</u>	3 Vrms 150 KHz to 80 MHz <u>6 V in ISM bands</u> <u>between 0,15</u> <u>MHz and</u>	Portable and mobile RF communications equipment should be used no closer to any part of the product including cables, than the recommended separation distance calculated from the equation applicable to

	<u>MHz and</u> <u>80 MHz</u> <u>80 % AM at 1</u> <u>kHz</u>	<u>80 MHz</u> <u>80 % AM at 1</u> <u>kHz</u>	the frequency of the transmitter.
Radiated RF IEC 61000-4-3	3 V/m <u>80MHz to 2,7</u> <u>GHz</u>	3 V/m <u>80MHz to 2,7</u> <u>GHz</u>	Recommended separation distance: $d = 1,2 \sqrt{P}$ $d = 1,2 \sqrt{P}$ 80MHz to 800 MHz $d = 2,3 \sqrt{P}$ 800MHz to 2,7GHz Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in metres (m).
			Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey, ^a should be less than the compliance level in each frequency range. ^b
			Interference may occur in the vicinity of equipment marked with the following symbol:
			
NOTE1 At 80 MHz and 800 MHz, the higher frequency range applies. NOTE2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.			

- a Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the product is used exceeds the applicable RF compliance level above, the product should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the product.
.
- b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3V/m.


Recommended separation distance between portable and mobile RF communications equipment and the product			
The product is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the product can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the product as recommended below, according to the maximum output power of the communications equipment.			
Rated maximum output power of transmitter W	Separation distance according to frequency of transmitter m		
	150 kHz to 80 MHz $d = 1,2\sqrt{P}$	80 MHz to 800 MHz $d = 1,2\sqrt{P}$	<u>800 MHz to 2,7 GHz</u> $d = 2,3\sqrt{P}$
0,01	0,12	0,12	0,23
0,1	0,38	0,38	0,73
1	1,2	1,2	2,3
10	3,8	3,8	7,3
100	12	12	23
For transmitters rated at a maximum output power not listed above, the recommended separation distance d in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where p is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer. NOTE1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies. NOTE2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.			

IV. Installation

A. Assembly


Standard Column

1. Fasten and tighten four screws at the bottom of the base. Ensure four adjustable feet and stability foot are at same level before using device.


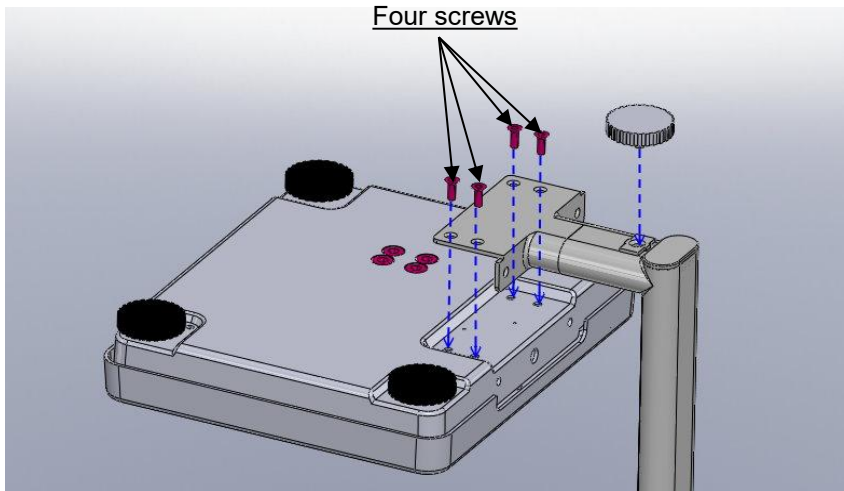


Castor wheel column


1. Fasten and tighten four screws at the bottom of the base

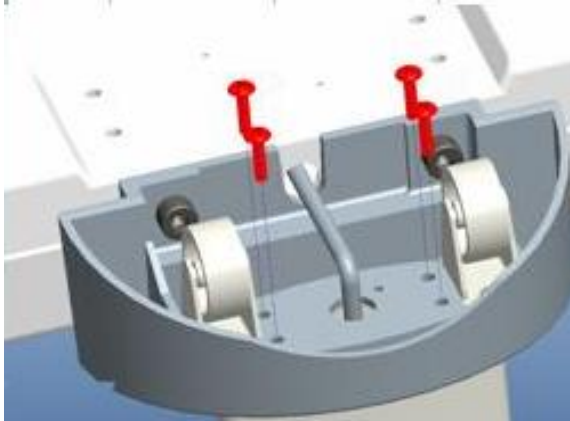


2. Ensure four adjustable feet and stability foot are at the same level before using the device. Rotate counter-clockwise to extend, clockwise to retract

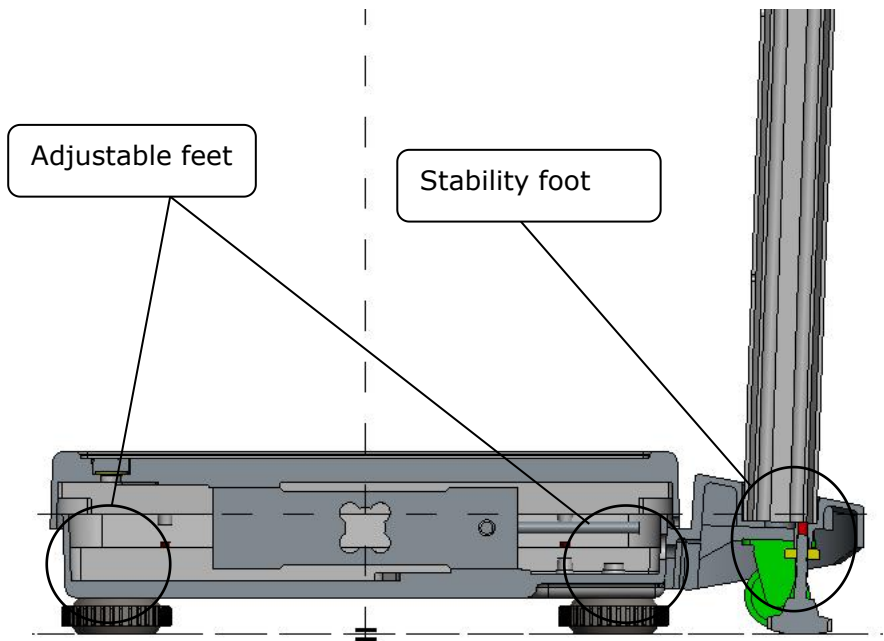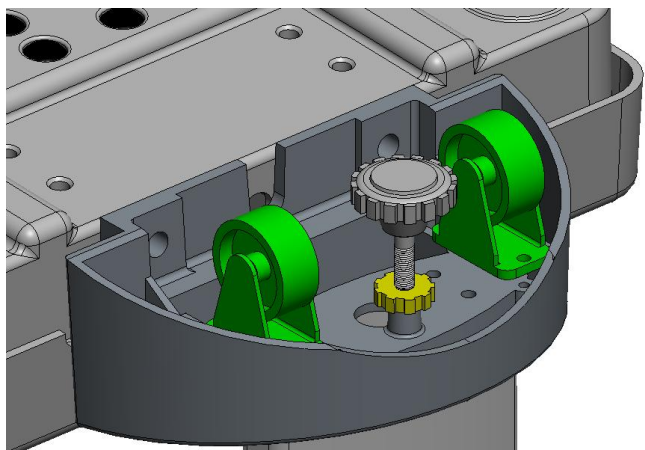


3. Retract stability foot before moving device using castor wheels

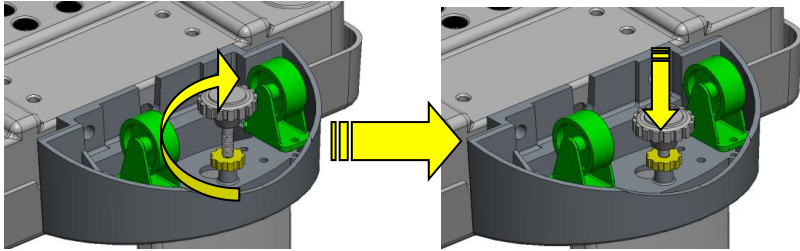

Note: rotate counter-clockwise to extend, clockwise to retract

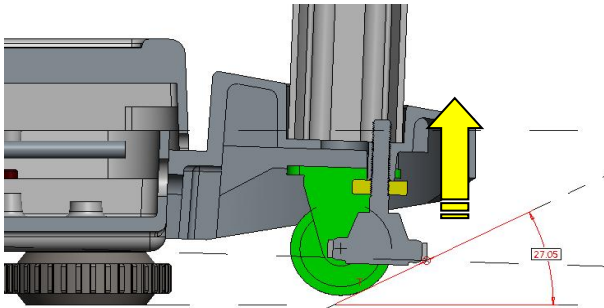


Ensure stability foot is retracted before using castor wheels


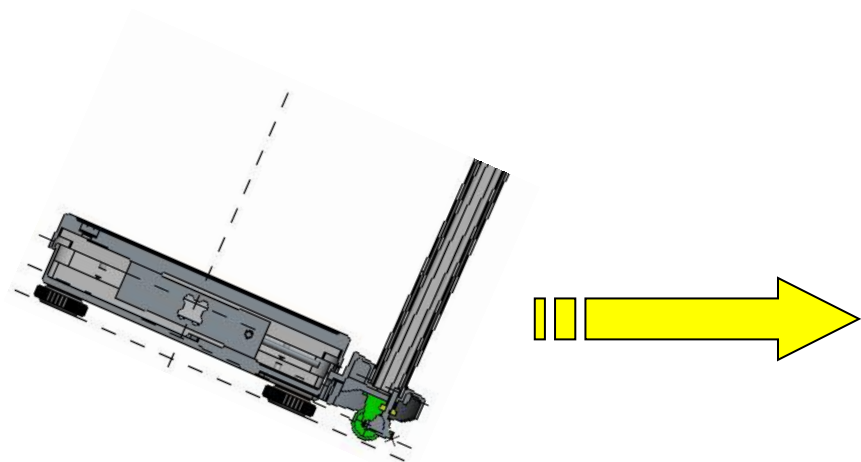


B. Inserting Batteries


1. Open battery housing cover

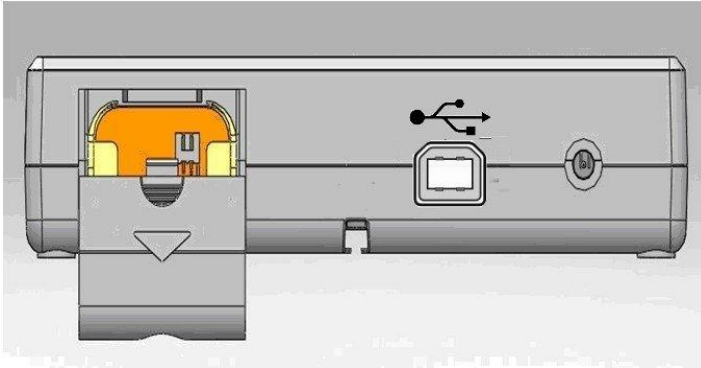


2. Accessing batteries

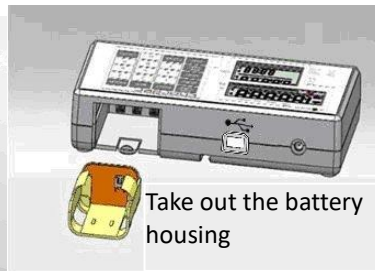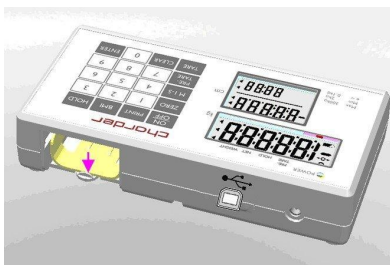


3. Use either rechargeable battery pack, or AA batteries

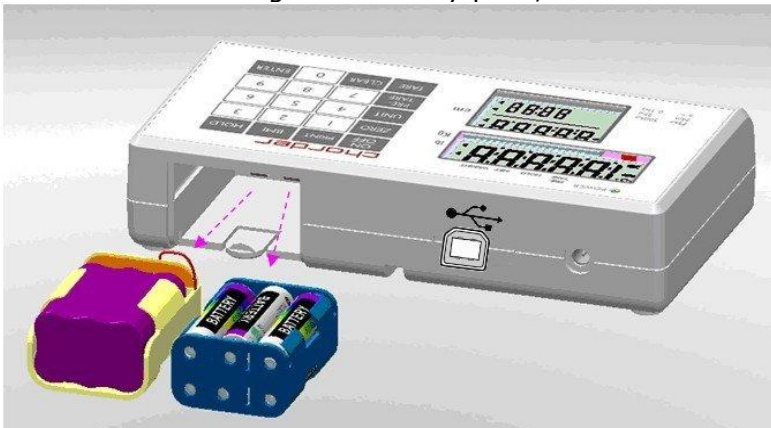


4. Ensure batteries are installed into the housing correctly

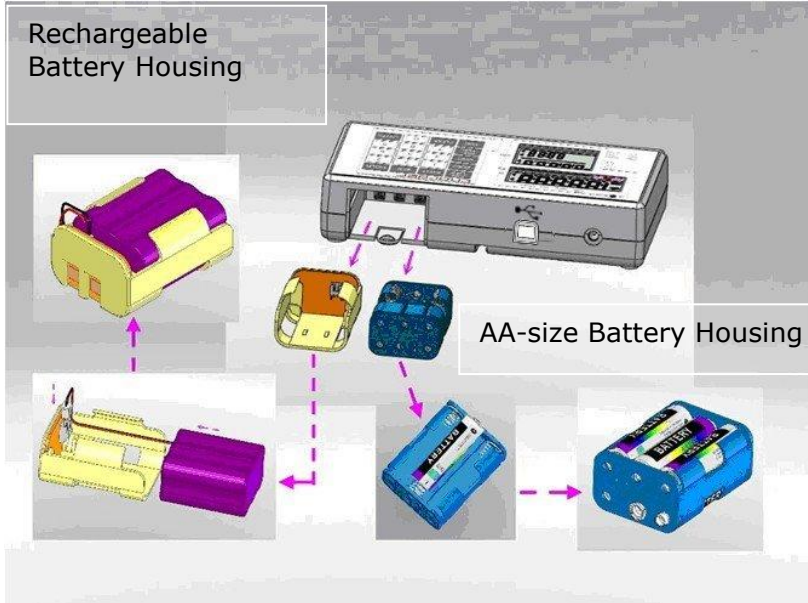

5. Install the battery housing into the compartment, and make sure the right side of housing pin is facing towards inside of the connecting position

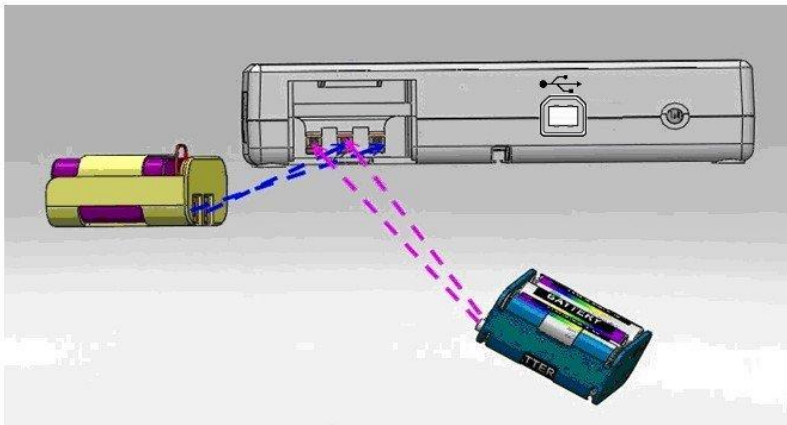

6. Slide back the cover to close the battery housing compartment. Turn on power to confirm that battery is correctly installed.

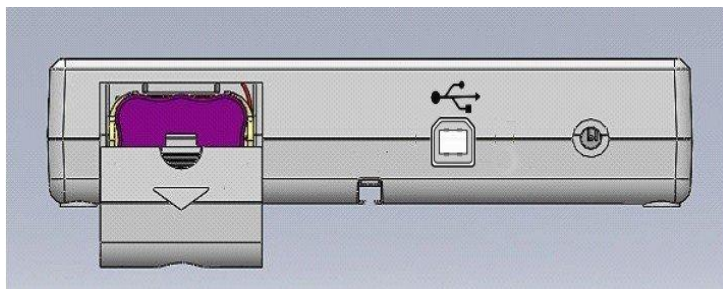


Using Rechargeable Battery (optional)

The rechargeable battery should be recharged at least once every 3 months, regardless of if the device has been used. Battery can be charged by plugging device's exclusive adapter into AC Connector Port.

After a long period in storage (e.g. >3 months), the battery should run a full cycle (charge/discharge) to allow it to restore full capacity.

Ensure rechargeable battery housing is installed and inserted properly into the compartment.

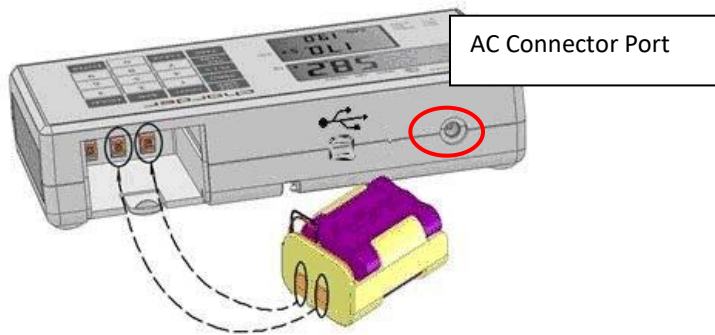


If Lo prompt displays on the LCD, please charge battery promptly to avoid battery damage.

C. Using Adapter


1. Connect adapter to indicator before connecting to mains power supply
2. Disconnect adapter from mains power supply before unplugging adapter pin from indicator.

D. Attaching Height Rod to Column

Standard (Narrow) Column

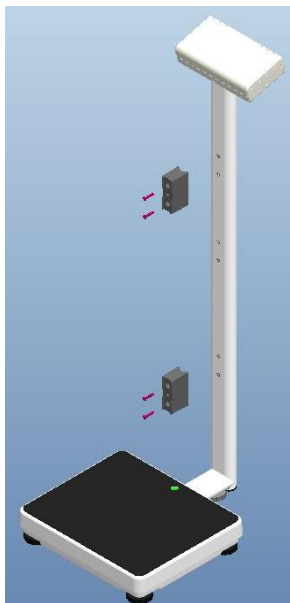

Step 1. Attach two fixing blocks to column using four flat-head screws

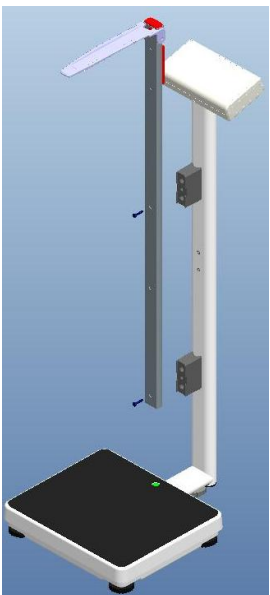


Step 2. Attach height rod to blocks using two flat-head screws

Item	Name	Quantity
1	Fixing block screws	4
2	Fixing blocks	2
3	Height Rod to fixing block screws	2

* Photo of display for reference only. Please refer to the actual product.


Castor Wheel Column

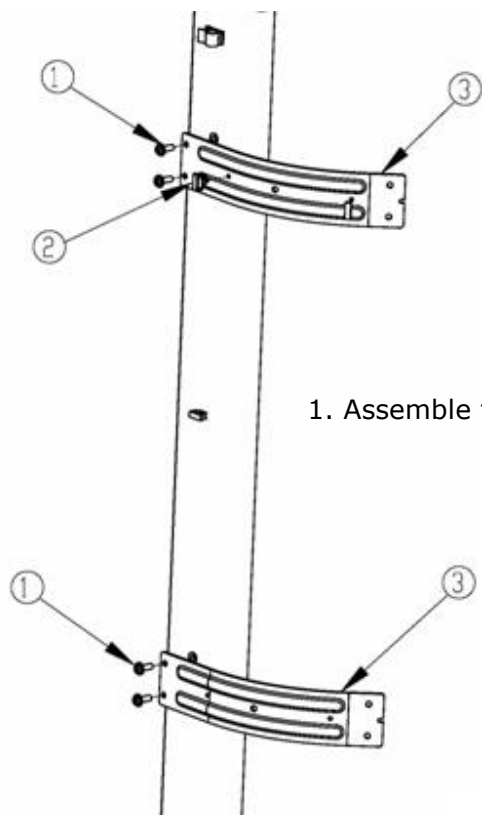

1. Assemble two brackets on the column

Item	Name	Quantity
1	M5x0.8x11 round head screw	4
2	Relief Bushing	2
3	Bracket for HM200D/HM201D/HM201M	2

* Photo of display for reference only. Please refer to the actual product.

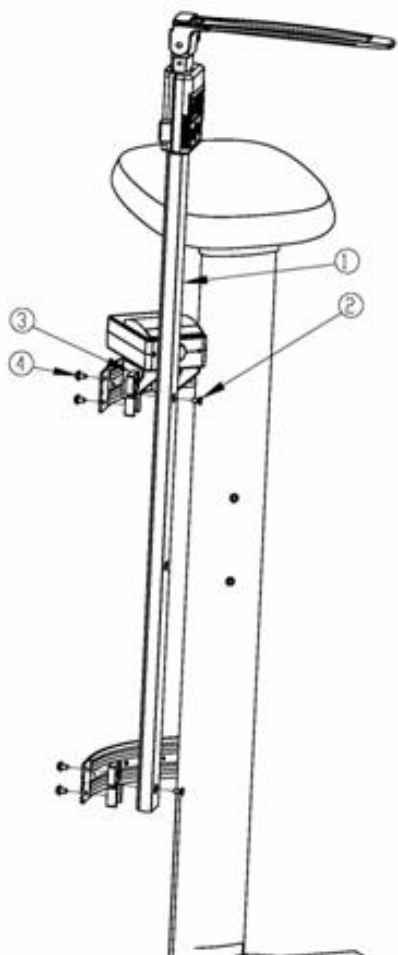


2. Attach Height Rod to bracket and tighten screws.

Item	Name	Quantity
1	Height Rod (Compatible with: HM200D/HM201D/HM201M)	1
2	M5x10L flat head screw	2
3	Fixing block	2
4	M5x0.8x11	4

* Photo of display for reference only. Please refer to the actual product.


Connecting height rod to indicator (HM200D/HM201D)

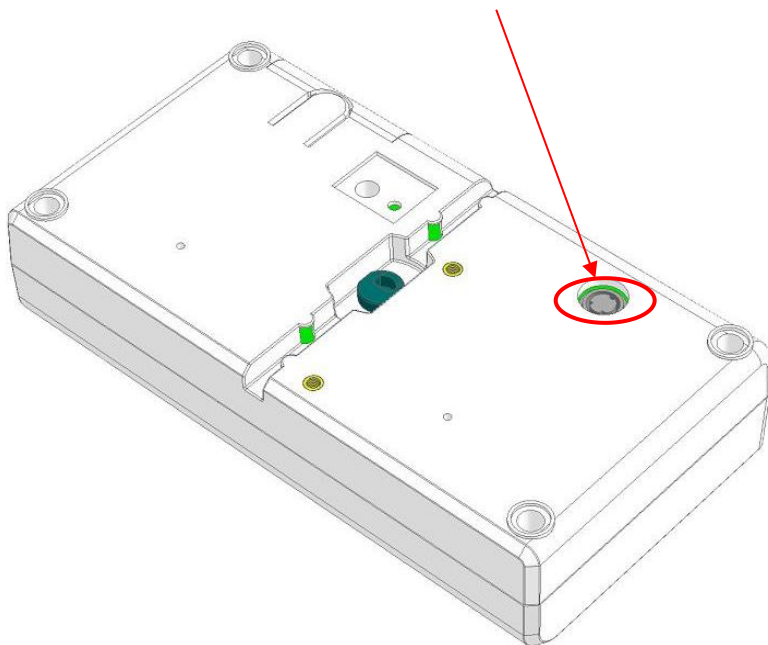

Digital height rod data transmission port on indicator


E. Attaching Thermal Printer

Standard (Narrow) Column

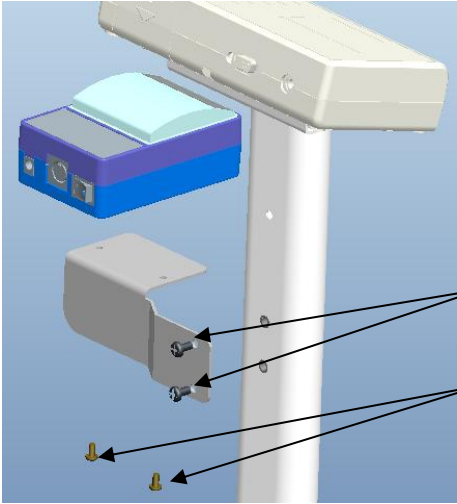


Washer head screw M5*0.8*15mm

Cross head screw M4*0.7*6mm

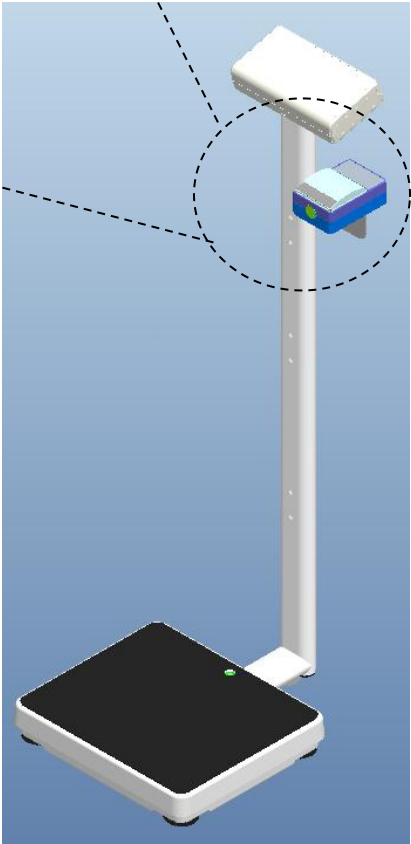

Castor Wheel Column

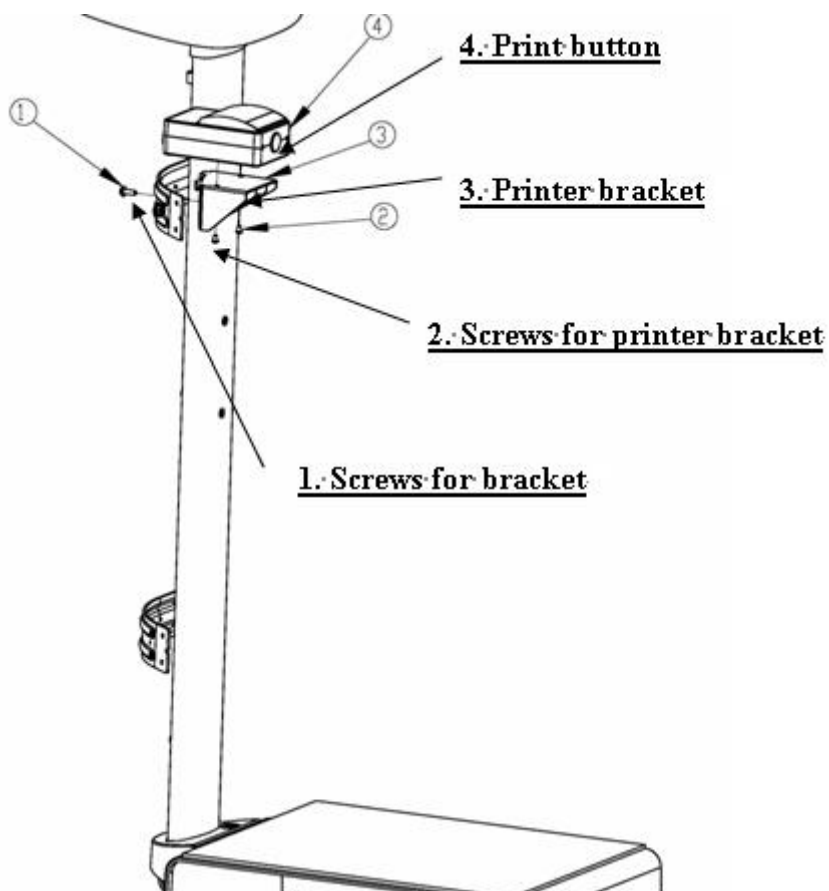


Item	Parts	Qty
1	M5*15L head screw	1
2	Screws for printer bracket	2
3	Printer bracket	1

1. Install the side bracket



2. Install the thermal printer on the bracket

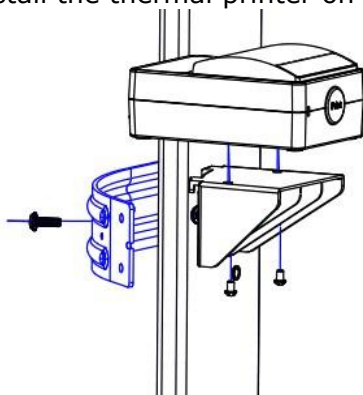

V. Indicator

A. Indicator and Key Functions



(Wireless functionality optional)

Key Function

1. **ON/OFF**: Power on or power off.
2. **ZERO**: Reset display to 0.0 kg display (can be used if within $\pm 2\%$ of full capacity). Press and hold for 3 seconds to enter device settings.
3. **M1-5**: Saving pre-tare values (up to 5)
4. **PRE-TARE**: Pre-tare the known weight of an object (ex: chair) before beginning measurement.
5. **TARE**: Allows user to deduct weight from reading after measurement
6. **PRINT**: When printer or PC is connected to the scale, press this key to print results
7. **BMI**: Calculation of Body Mass Index
8. **HOLD**: Determine stable weighing value - used when weight is unstable. Press and hold for 3 seconds to enter time setting.
9. **0-9**: For entering digits.
10. **CLEAR**: Clear incorrect data input.
11. **ENTER**: Confirm input.

B. Display layout



Unit of height (cm)
Indicates that the height is shown in centimeters

BMI
Body Mass Index is a height to weight ratio, and is calculated by the following formula




Definitions

Stable symbol: Indicate that weight is stable.

Zero symbol: Weight is at zero

Minor weight: Weight under zero.

Low battery: Battery needs to be charged or replaced.

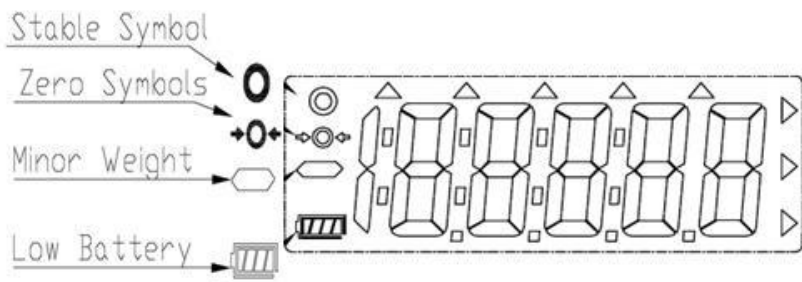

VI. Using Device

A. Basic Operation

Switch on the device using **[ON/OFF]** key. The device will automatically perform self-calibration, displaying software version.

Once "0.00 kg" appears on indicator, device is ready for measurement.

Note: If "0.00 kg" does not display on indicator, press **[ZERO]** key to zero the device. This function can be used for weight within $\pm 2\%$ of full capacity.

Guide subject to stand upon the measurement platform. After the weight has stabilized, the "stable" symbol will appear on indicator.

Note: If subject's weight exceeds scale capacity (300 kg, including tare), indicator will display "Err" prompt due to overload.

B. Hold

The hold function determines average weight, designed to be used if subject's weight will not stabilize (ex: an active child).

Note: if fluctuation is too severe, average weight determination will be difficult and hold may not function correctly

1. Switch on the device normally.
2. Press the **[HOLD]** key. "HOLD" will be displayed on the indicator.
3. Guide subject to stand on measurement platform.
4. After a few seconds, the average weight will be displayed on the indicator. This weight will be locked - at this point, subject can step off from device.
5. To release the locked weight, press the **[HOLD]** key again to return to the device to normal mode.

Note: Hold function can be activated before or after subject stands on measurement platform. However, if subject finds it difficult to stand still, we recommend activating Hold after subject stands on platform.

C. BMI

1. In normal mode, press the **[BMI]** key to enter BMI mode.
2. Display will show last recorded height. Left-most digit will flash.
3. Enter height using numeral keys (ex: 170 cm). Input will automatically move to next digit. Press **[CLEAR]** key to re-input. Press **[TARE]** key to manually move to next digit.
4. After inputting height, press **[ZERO]** to confirm.
5. Proceed to weigh subject as usual. Indicator will display weight, height, and BMI.

NOTE: Hold function can be used at this time if weight is unstable

6. Press **[BMI]** key to return to normal mode.

BMI (w/HM200D or HM201D)

1. Ensure HM200D/HM201D is plugged into indicator.
2. In normal mode, press the **[BMI]** key to enter BMI mode.
3. Proceed to weigh subject as usual. Indicator will display weight, height, and BMI.
4. Lower stopper on HM200D/HM201D until it touches top of subject's head. Device will automatically calculate BMI based on change in height and weight.

NOTE: Hold function can be used at this time if weight is unstable

5. Press **[BMI]** key to return to normal mode.

Category	BMI (kg/m ²)	Risk of obesity-related disease
Under	< 18.5	Low
Normal	18.5-24.9	Average
Over	24.9-29.9	Slightly Increased
Obese I	30.0-34.9	Increased
Obese II	35.0-39.9	High
Obese III	> 40	Very High

(World Health Organization adult BMI standards)

D. Tare

The tare function allows the user to deduct the weight of objects from the device's measurement result.

1. Place object that needs to be tared onto measurement platform.
2. Press **[TARE]** key after stable symbol appears on indicator. Display will indicate "0.00 kg".
3. Guide subject (plus tared object) to be weighed upon measurement platform. Conduct measurement.
4. To clear tare value, remove all objects from measurement platform, and press **[TARE]** key.

E. Pre-Tare

The Pre-Tare function is used to subtract the known weight of a substance prior to weighing. The MS4910 can store 5 sets of pre-tare values.

Pre-tare values can be stored using two different methods: "Load Weight", or "Input Manually".

After pre-tare weights have been stored, they can be recalled by holding the **[PRE-TARE]** key for 3 seconds.

A. Load Weight

DESCRIPTION	EXAMPLE
Press M1-5 key after loading weight on the platform; the indicator will display blinking "m" symbol.	
Press numeral key 1 ~ 5 to assign this number with the current pre-tare weight.	
Press [ENTER] key to store pre-tare weight; the indicator will make a beep sound.	

B. Input Manually

DESCRIPTION	EXAMPLE
Press [PRE-TARE] key. Left-most digit will begin blinking. If no further action is taken within 6 seconds, indicator will return to normal mode	
While digit is blinking: Enter pre-tare weight using 0~9 keys. Ex: to pre-tare 5.0 kg of weight, press 0-0-5-0. Ex: to pre-tare 13.5 kg of weight, press 0-1-3-5. Press [ENTER] key to confirm the pre-tare weight.	
Indicator will display minus sign to the left of pre-tare weight value.	

To save this pre-tare weight value in memory:

Press M1-5 key; the blinking "m" symbol will appear on the display.



Press numeral key 1 ~ 5 to assign this number with the current pre-tare weight.



Press **[ENTER]** key to store pre-tare weight; the indicator will make a beep sound.



C. Recall Pre-Tare Weight

DESCRIPTION	EXAMPLE
Press and hold [PRE-TARE] key for 3 seconds. Indicator will display pre-tare value M1 first. The pre-tare value will flash.	
Press numeral keys 1 ~ 5 to choose pre-tare value	
Press [ENTER] key to confirm which pre-tare weight to select; the device will automatically deduct pre-tare weight.	
Press [CLEAR] key to return to Normal Mode	

NOTE: Pre-tare weight must be under max capacity, otherwise screen will show 0.00 after **[ENTER]** key is pressed, and the operator will have to re-input pre-tare settings.

F. Print


If thermal printer is connected to indicator, results can be printed by pressing **[PRINT]** key.

VII. Device Setup

A. Setting Time & Date

Press and hold **[HOLD]** key for 3 seconds to enter Time Setting mode.

Example: Inputting 2008, Dec 25, 8:00am

	Year Setting Enter year using numeral keys 0-9. Press [HOLD] key once completed to proceed to month & day setting.
	Month & Day Setting. Enter month, followed by day using numeral keys 0-9. Ex: December 25th is "12.25". Input 1-2-2-5. Press [HOLD] key once completed to proceed to time setting.
	Time Setting Enter time (24hr format) using numeral keys 0-9. Ex: 08:00am is input by pressing 0-8-0-0. Press [HOLD] key once completed to confirm time settings and proceed to confirmation.
	Device will display new time and date settings, cycling between year, month & day, and time. YYYY→MM.DD→:HH:MM Press [HOLD] key to return to normal weighing mode.

B. Device Setup

When the device is switched on, press and hold the **[ZERO]** key for about 3 seconds, until the display shows the "SETUP", followed by "A.OFF" (first option in setting menu).

In device setup menu:

[TARE] to toggle next menu option

[ZERO] to toggle previous menu option

[HOLD] to confirm selection / enter submenu

A_OFF

Auto Power-Off: Instruct device to shut off automatically after a certain period of time.

Auto off options: 120 sec / 180 sec / 240 sec / 300 sec / off

Press **[HOLD]** to toggle between time options, and **[TARE]** to confirm selection.

bUrr

Buzzer/Beep:

When function is turned on, beeping noise will be made when: indicator is turned on, keys are pressed, and weight is stable.

Press **[HOLD]** to toggle between on/off, and **[TARE]** key to confirm selection.

HoLdS

Hold Stop: When Hold Stop is "on", Hold will deactivate after subject leaves measurement platform.

Press **[HOLD]** to toggle between on/off, and **[TARE]** key to confirm selection

Language

Language: Set thermal printer language

Press **[HOLD]** to toggle between English, Italian and Polish.

Press **[TARE]** key to confirm selection.

Font

Font size: Set thermal printer font size.

Press **[HOLD]** to toggle between normal and double (larger).

Press **[TARE]** key to confirm selection.

BT / Wifi

BT / Wifi (optional) : If device has BT or Wifi module installed, the function can be turned OFF/BT/Wifi.

Press **[HOLD]** to toggle between OFF/BT/Wifi, and **[TARE]** to confirm selection.

Wi-Fi Setting

Wi-Fi Setting (optional): If device has Wi-Fi module installed, this option will appear.

Press **[HOLD]** to toggle between "Auto" and "PKEY". Press **[TARE]** to confirm selection.

If "Auto" is selected, weight measurement will be automatically sent to connected printer or device. If "PKEY" is selected, transfer will occur manually only after **[PRINT]** key is pressed.

VIII. Setup USB Connection to PC

For successful connection, PC hardware connected to device must be compatible with USB 2.0 or above. Operators should select a USB cable length that is most suitable to the operating environment.

1. Charder Smart Data Manager can be used to connect the device to a PC. The software program can be downloaded from the Charder website:

[LINK URL]

<https://www.chardermedical.com/download.htm>

2. Connect USB cable to device indicator and PC. Follow installation instructions.

Program Setup

1. After installation of Charder Smart Data Manager is complete, software will automatically search for COM port. Press **[Connect]**. Once connected, **[Connect]** button will change to **[Disconnect]**.

The screenshot displays the Charder Smart Data Manager software interface. At the top, the title bar reads "Charder Smart Data Manager". Below the title bar, there is a dropdown menu for the COM port, currently set to "COM 1", and a "Connect" button. The main area of the interface contains several input fields for patient data, arranged in two columns. The left column includes fields for Gross Weight (0.0 kg), Tare Weight (0.0 kg), Net Weight (0.0 kg), Height (0.0 cm), BMI (0.0), and a Data section with "Auto" and "Manual" buttons. The right column includes fields for First Name (Enter), Last Name (Enter), Patient ID (Enter), Date of Birth (31 / 12 / 1990), and Gender (Male/Female). At the bottom of the interface, there are three buttons: "Collect", "Clear", and "Save as". A small text box at the bottom left says "Please press 'Connect'." and "Update Time: Model:".

Conducting Measurement

1. Input subject's first name, last name, patient ID, date of birth (DD/MM/YYYY), gender, and height (for BMI calculation) into software if needed. Press **[Clear]** to clear all input.

NOTE: information can also be input after weight measurement.

Chorder Smart Data Manager COM [Connect] - [X]

Gross Weight	0.0	kg
Tare Weight	0.0	kg
Net Weight	0.0	kg
Height	167.0	cm
BMI	0.0	

Data [Auto] [Manual]

Please press "Connect".
Update Time:
Model:

First Name Jane
Last Name Doe
Patient ID 20190201
Date of Birth 31 / 12 / 1965
Gender [Male] [Female]

[Collect] [Clear] [Save as] [?]

2. Conduct measurement. If **[Auto]** is selected, results will be transmitted from device to software automatically and displayed on the left of screen. If **[Manual]** is selected, user must press "Collect".

Chorder Smart Data Manager COM [5] [Disconnect] - [X]

Gross Weight	72.5	kg
Tare Weight	0.0	kg
Net Weight	72.5	kg
Height	167.0	cm
BMI	26.0	

Data [Auto] [Manual]

Data updated:
Update Time: 06/03/2020 11:40:05
Model:

First Name Jane
Last Name Doe
Patient ID 20190201
Date of Birth 31 / 12 / 1965
Gender [Male] [Female]

[Collect] [Clear] [Save as] [?]

Saving & Printing Results

1. Press **[Save as]** to save measurement results as .csv file on PC. Default file name is same as user ID. (ex: 20190201.csv) To track changes and multiple measurements for the same subject, we recommend not changing the default file name.

Chorder Smart Data Manager COM [5] Disconnect

Gross Weight 72.5 kg First Name Jane

Tare Weight 0.0 kg Last Name Doe

Net Weight 72.5 kg Patient ID 20190201

Height 167.0 cm Date of Birth 31 / 12 / 1965

BMI 26.0 Gender Male Female

Data Auto Manual

Data updated:
Update Time: 06/03/2020 11:40:05
Model:

Collect Clear Save as

2. Result example:


	A	B	C	D	E	F	G	H	I	J
1	Patient ID	First Name	Last Name	Date of Bi	Gender	Gross Weig	Tare Weight	Net Weight	Height	BMI
2	20190201	Jane	Doe	31/12/1965	Male	72.4 kg	0.0 kg	72.4 kg	167.0 cm	26
3										
4										
5										

If previous results were saved in "20190201.csv", new results also need to be saved as "20190201.csv" (overwriting old file) in order to save multiple results for the same subject.

	A	B	C	D	E	F	G	H	I	J
1	Patient ID	First Name	Last Name	Date of Bi	Gender	Gross Weig	Tare Weight	Net Weight	Height	BMI
2	20190201	Jane	Doe	31/12/1965	Male	72.4 kg	0.0 kg	72.4 kg	167.0 cm	26
3	20190201	Jane	Doe	31/12/1965	Male	75.2 kg	0.0 kg	75.2 kg	167.0 cm	27
4										

Results will be saved in chronological order of measurement.

3. Press the printer icon to print out result using a printer connected to the PC.

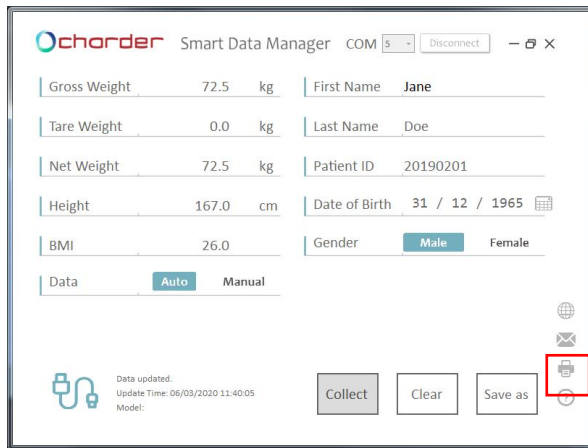


Chorder Smart Data Manager COM 5 Disconnect

Gross Weight	72.5 kg	First Name	Jane
Tare Weight	0.0 kg	Last Name	Doe
Net Weight	72.5 kg	Patient ID	20190201
Height	167.0 cm	Date of Birth	31 / 12 / 1965
BMI	26.0	Gender	Male Female
Data	Auto Manual		

Data updated:
Update Time: 06/03/2020 11:40:05
Model:

Collect Clear Save as

Printer icon highlighted with a red box.

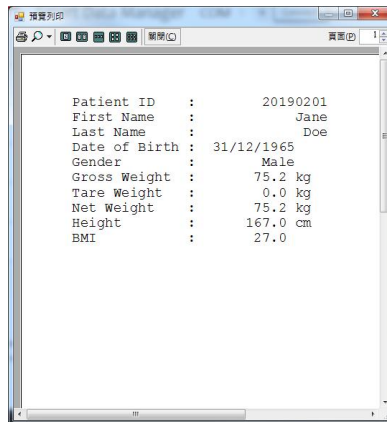

摘要打印

Print preview window showing the following data:

```
Patient ID : 20190201
First Name : Jane
Last Name : Doe
Date of Birth : 31/12/1965
Gender : Male
Gross Weight : 75.2 kg
Tare Weight : 0.0 kg
Net Weight : 75.2 kg
Height : 167.0 cm
BMI : 27.0
```

IX. Wireless Connection

If the device has the wireless or BT module installed, the indicator can transmit measurement results wirelessly. Please see Chorder wireless or BT software instructions for details.

X. Troubleshooting

Product Defects

Charder's warranty is effective for the original purchaser of this device, subject to the terms and conditions listed in the Warranty Program & Return Policy.

1. If Charder is responsible for a fault or defect present upon receipt of the unit, Charder shall either repair the fault, or supply a replacement unit. Should the repairs or replacement delivery fail, statutory provisions shall be valid. The period of warranty shall be two years, beginning on the date of purchase. Please retain your receipt as proof of purchase.

2. No responsibility shall be accepted for damage caused through any of the following reasons: unsuitable or improper storage or use, incorrect installation or commissioning by the owner or third parties, natural wear and tear, changes or modifications, incorrect or negligent handling, chemical, electrochemical, or electrical interference, unless damage is attributable to negligence on the part of Charder.

If device is not covered under warranty, a service maintenance charge will apply, plus cost of replacement parts.

Before contacting your local Charder distributor for repair service, we recommend considering the following troubleshooting procedures:

Self-inspection

1. Device will not power on

- If battery power is depleted, replace with new batteries
- If batteries are not used, check if the power adapter is plugged into the device properly. Check if power adapter is plugged into mains properly

2. Indicator showing "0000" ZERO SPAN out of range

- Interference due to factors such as RF disturbance or ground vibration. Relocate device to location without interference and try again
- Unstable platform feet - adjust platform feet according to bubble level indication (clockwise to retract, counter-clockwise to extend) and try again
- External objects interfering with measurement platform. Clear platform of objects and try again
- Device may not function properly on soft surfaces such as carpets or lawns. Relocate device to location with solid, stable floor
- If the steps above cannot resolve the problem, re-calibration may be required to correct weighing accuracy

3. Connection failure for data transmission to PC or printer

- Ensure wires are connected correctly between indicator and PC or printer
- Ensure printer is supplied with power. Ensure PC software is set up properly as indicated in this manual

Distributor support required

If the following errors occur, we recommend contacting your local Charde distributor for repair or replacement services:


1. Device will not power on

- Faulty on/off key
- Broken or damaged wires causing short circuit or faulty connection
- Safety fuse burnout
- Faulty adapter

2. Indicator damage

- Possible hardware defects include: uneven brightness in LCD screen, blurred text, smeared rainbow screen, incorrect decimal display
- Unable to save or read data
- Indicator shows "ERRL" after device is switched on
- Keys not responding
- Buzzer malfunction

Error Messages

Error Message	Reason	Action
	Low battery warning Voltage of battery is too low to operate device	Replace batteries, or plug in adapter
	Overload Total load exceeds device's maximum capacity	Reduce weight on measurement platform and try again
	Counting Error (too high) Signal from loadcells too high	Error normally caused by faulty loadcell or wiring. Please contact distributor
	Counting Error (too low) Signal from loadcells too low	Error normally caused by faulty loadcell or wiring. Please contact distributor
	Zero count over calibration zero range +10% while power on	Re-calibration required. Please contact distributor
	Zero count under calibration zero range -10% while power on	Re-calibration required. Please contact distributor
	Program Error Fault with device software	Error normally caused by faulty loadcell or wiring. Please contact distributor

XI. Product Specifications

A. Device Information

Model		MS4910
Display		DP3710
Weight Measurement	Capacity	300 kg x 0.1kg
	Accuracy	±1.5e
	OIML	Class III
	LCD Screen	1.0-inch LCD screen (5 1/2 digits)
Dimensions (Standard)	Overall	360(W) x 480(D) x 1100(H) mm
	Platform	360(W) x 310(D) x 70(H) mm
	Column	1026 mm
	Device Weight	8.2 kg
Dimensions (Castor Wheel)	Overall	360(W) x 440(D) x 970(H) mm
	Platform	360(W) x 310(D) x 70(H) mm
	Column	850 mm
	Device Weight	7.8 kg
Key Functions		On/Off, Zero, Print, BMI, Hold, Pre-Tare, Tare, Clear, Enter, 0~9, M1-5
Data Transmission		USB, Wireless Module (optional) NOTE: Device should be connected to network by qualified distributors only.
Power Supply		Rechargeable battery pack (optional) or 6 AA batteries / Power adapter


Operation Environment	0°C~+40°C 15% / 85% RH 700 hPa ~1060 hPa
Optional Accessories	Thermal Printer, Height Meter
Standard Accessories	User manual x 1; Power Adapter x 1; USB cable x 1, M6*20 Screws x 4 M4*20 Screws x 4 (castor wheel)

B. Power Adapter Standards



Warning

The device is only compatible with the power adapters specified in the dashed block below.

AMP VOLTAGE	DRAWING NO.	CE APPROVED TYPE NO. / MODEL NO.	TYPE	Adapter plug
12V 2A	CD-AD-00041	UES24LCP-120200SPA	US	 90 - degree
	CD-AD-00041	UES24LCP-120200SPA	EU	
	CD-AD-00041	UES24LCP-120200SPA	UK	
	CD-AD-00041	UES24LCP-120200SPA	AU	

This image shows a single page of white paper with horizontal ruling lines. The lines are evenly spaced and run across the width of the page. There are no margins, text, or other markings on the paper.

This image shows a single sheet of white paper with horizontal ruling lines. The lines are evenly spaced and run across the width of the page. There are no margins, text, or other markings on the paper.

[illegible]

XII. Declaration of Conformity

This product has been manufactured in accordance with the harmonized European standards, following the provisions of the below stated directives:

	(EU) 2017/745 Regulation on Medical Devices
	2014/31/EU Non-automatic Weighing Instruments Directive (OIML models only)

RoHS Directive 2011/65/EU and Delegated Directive (EU) 2015/863

Radio Equipment Directive 2014/53/EU

(applicable if wireless module is used)

Part 15 of the Federal Communications Statement Rules

This device may not cause harmful interference.

This device must accept any interference received, including interference that may cause undesired operation.

Please see separate document showing on sticker of device for above markings.

Authorized EU Representative:



Obelis s.a.

Bd Général Wahis, 53
B-1030 Brussels
Belgium

Manufactured by:



Charder Electronic Co., Ltd.
No.103, Guozhong Rd., Dali Dist.,
Taichung City 41262 ,Taiwan

CD-IN-1269 [14214N] 08/2024